Digital-Control DC Power Supply

KD3000-6000 Series User Manual

KORAD

User Manual

Main Features

Low noise
Cooling fan controlled by
Heatsink temperature
Constant voltage / constant
Digital panel control
4 digits display
Software calibration
Over Current Protection
Button lock function

SAFETY INSTRUCTION

Safety Guidelines

- •Do not block or obstruct the cooling fan vent opening.
- Avoid severe impacts or rough handling that leads to damage.
- ·Do not discharge static electricity.
- Do not disassemble unless you are qualified as service personnel.

AC INPUT



- •AC Inut Voltage: 110V / 120V / 220V / 230V , 50 / 60 Hz
- Connect the protective grounding conductor of the AC power cord to an earth ground, to avoid electrical shock.

Operation Environment

- Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (note below)
- Relative Humidity: < 80%
- ·Altitude: < 2000m
- Temperature: 32 104°F

Storage environment


- Location: Indoor
- •Relative Humidity: < 70%
- •Temperature:-10-70°C


FUSE



Model	110/120 VV	220/230 V
KD3003D	T4A/250 V	T2A/250 V
KD3005D	T5A/250V	T3A/250 V
KD6003D	T5A/250V	T3A/250 V
KD6005D	T10A /250V	T5A/250V


- To ensure fire protection, replace the fuse only with the specified type and rating.
- ·Disconnect the power cord before fuse replacement.
- Make sure the cause of fuse blowout is fixed before fuse replacement.

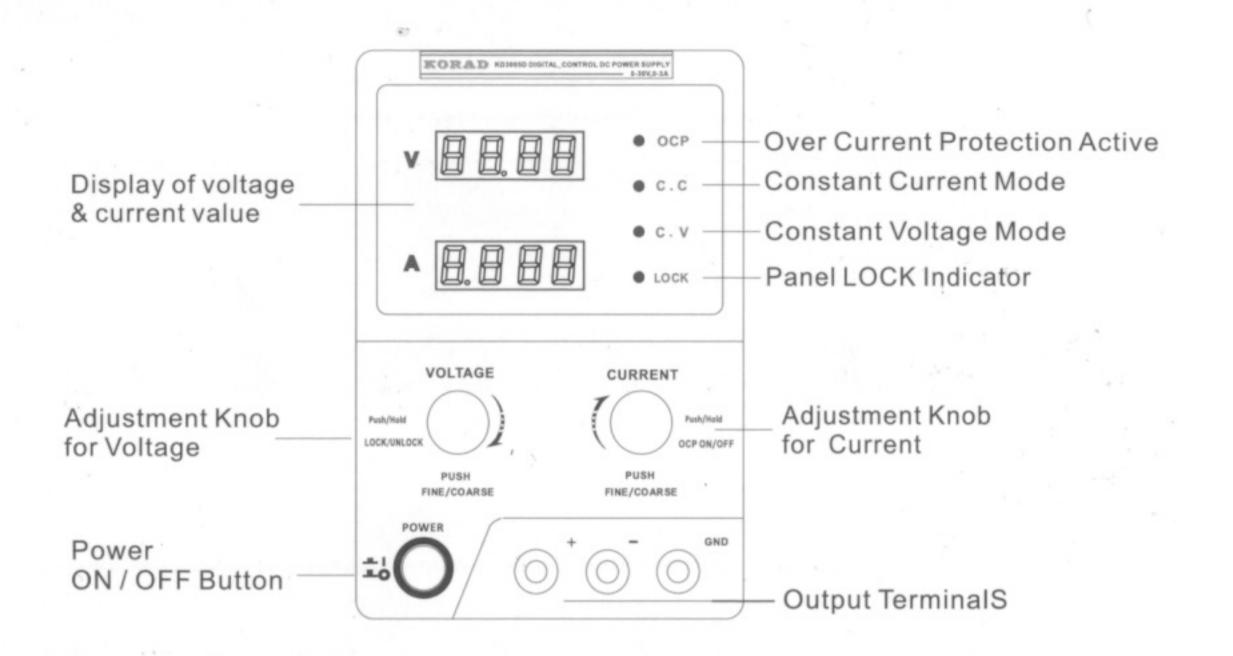

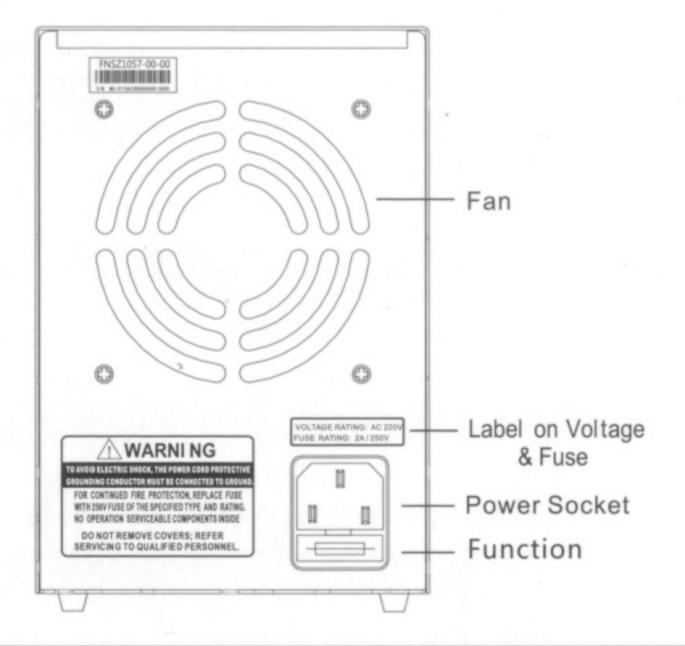


DISPLAY

Voltage level v



Voltmeter displays the setup value of output voltage .

Current level A



Displays the setup value of output current .


Condition Indicators - LED Panel Lights

- OCP Over Current Protection indicator. When the power supply is in OCP mode this light is on.
- C.C indicates constant current. When the power supply is in constant current mode, this light is on.
- C.V indicates constant voltage. When the power supply is in constant voltage mode, this light is on.
- LOCK
 Panel LOCK Indicator

Voltage and Current Adjustment Knob Operation


There are 2 adjustment modes for the voltage and current digits, that is, Mode 1 and Mode 2. Mode 1: Before setting, push the knobs to adjust the voltage and current digits. Mode 2: adjust directlu, no need to pust the knobs. And these 2 modes can be shifted by pushing the voltage adjustment knob and the current adjustment knob at the same time and holding for 2 seconds.

Mode 1



FINE/COARSE


Voltage Adjustment Knob: Push the voltage adjustment knob and then the voltage meter will flicker, when voltage output can be changed by adjusting the knob. Then the resolution of the knob rotation can be changed. Push it to change the resolution of voltage adjustment;



Current Adjustment Knob: Push the voltage adjustment knob and then the voltage meter will flicker, when voltage output can be changed by adjusting the knob. And push the knob again when the meter flikers, then the resolution of the knob rotation can be changed.


Mode 2

In mode 2, rotate the adjustment knobs to adjust the voltage and current values. The default of the voltage initial settings is 1v while that of the current is 100mA. The voltage and current digits can be changed by pushing the knobs.



Operation of LOCK Function

press and hold for 3 seconds to lock the front panel and then press again and hold for 3 seconds to unlock the panel.



FINE/COARSE

Operation of Over Current Protection

press and hold for 3 seconds to start OCP mode, where the output will be cut off when the output current reaches the set value. In the OCP mode, rotate this knob to recover the output. Press and hold for 3 seconds again and then the OCP function will be closed.

Power Switch and Output Terminals

On / Off main power.

to outputs voltage and current.

Connects the ground (earth) terminal.

KORAD

Specifications

Note: The specifications below are tested under the conditions of temperation 25℃+-5℃ and the warm-up for 20 minutes.

Models	KD3003D	KD3005D	. *KD6003D	KD6005D
Voltage	0-30V	0-30V	0-60V	0-60V
Current	0-3A	0-5A	0-3A	0-5A
Load Re	gulation			
-	≤0. 01%+2mv ≤0. 1%+5mA	≤0. 01%+2mv ≤0. 1%+10mA	≤0. 01%+2mv ≤0. 1%+5mA	≤0.01%+3mv ≤0.1%+3mA
Line Re	gulation			
	≤0. 01,%+3mv ≤0. 1%+3mA	≤0. 01%+3mv ≤0. 1%+3mA	≤0. 01%+3mv ≤0. 1%+3mA	≤0. 01%+3mv ≤0. 1%+3mA
Setup R	esolution			
Voltage Current	10m V 1mA	10m V 1mA	10m V 1mA	10m V 1mA
Setup A	ccuracy (25°C	+-5°C)		
Voltage Current	≤0.5%+20mV ≤0.5%+5mA	≤0.5%+20m V ≤0.5%+10m A	≤0.5%+30mV ≤0.5%+5mA	≤0.5%+30mV ≤0.5%+10mA
Ripple(2	20-20M)			
Voltage Current	≤1m∨rms ≤3mArms	≤2mVrms ≤3mArms	≤1mVrms ≤3mArms	≤1mVrms ≤3mArms
Temp. C	oefficient			
Voltage Current	≤150 ppm ≤150 ppm	≤150ppm ≤150ppm	≤150 ppm ≤150 ppm	≤150ppm ≤150ppm
Read Ba	ack Resolution			
Voltage Current	10 mV 1 mA	10 mV 1 mA	10mV 1mA	10m V 1m A
Read Ba	ack Temp. Coe	fficient		
Voltage Current	≤150 ppm ≤150 ppm	≤150 ppm ≤150 ppm	≤150 ppm ≤150ppm	≤150 ppm ≤150ppm
Accesso				
THE RESIDENCE OF THE PERSON NAMED IN		Power cord*1		
	and Dimension			
		3D, KD6005D: 110m .8Kg, KD6003D 4.9		

SHENZHEN KORAD TECHNOLOGY CO., LTD.

Address:F3, Building A4, District B, Songbai Industrial Park, Guangming New District, Shenzhen, 518106, P.R.China.

Tel: 86-755-61535026 Fax: 86-755-61535025

E-mail: adam@koradtechnology.com

www.koradtechnology.com

www.korad.com.cn